

Sample Received: **May 6, 2026**

COA Issued: **May 15, 2026**

PRODUCT INFORMATION

Vendor: HG Peptide Labs	Sample Name: Klow Blend 80mg	Sample Type: Blue lyophilized powder	Lot Number: NA	MW (g/mol): 342.1, 403, 1419.3, 4964
-----------------------------------	--	--	--------------------------	--

ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS




Purity: RP-HPLC (214 nm)

Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: Klow Blend	Klow Blend	MALDI-MS	✓ Conforms
Content	52.11, 10.67, 11.31, 10.91 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.6%	RP-HPLC (214 nm)	✓ Conforms

HPLC Chromatogram (Retention Time: 2.125, 2.53, 2.82, 6.08 min)

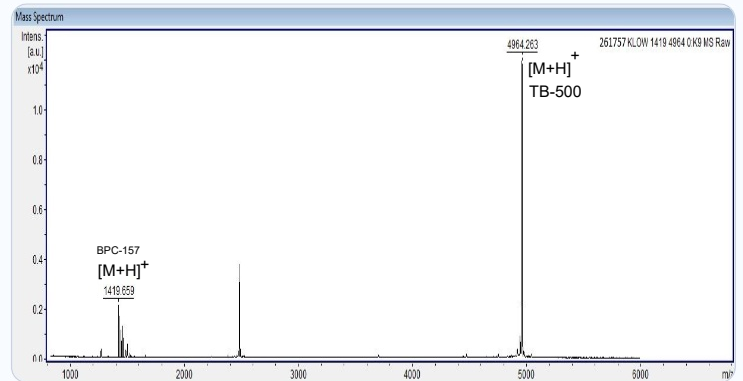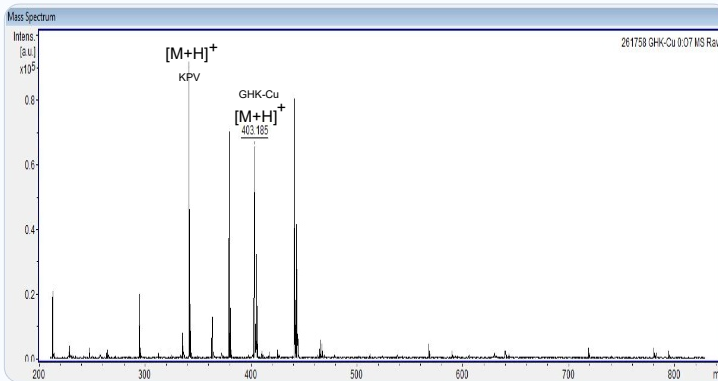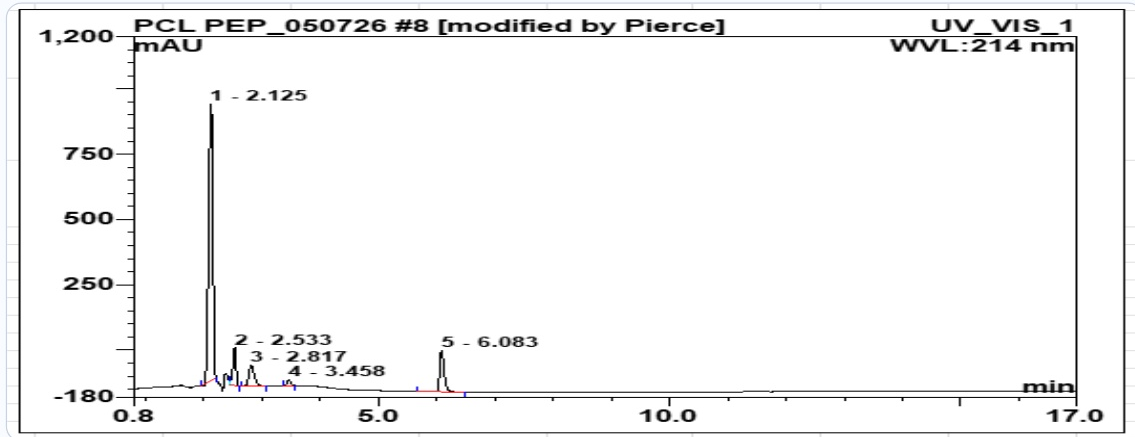

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: <https://bioviridians.com/coa-search.html>



Shane Straight

Shane Straight, M.S.

Principal Chemist, Bioviridian Inc.